



POSITIONING CHAIR
JUMBO™



USER MANUAL





Manufacturer takes responsibility for proper usage of the device only when the product was purchased from qualified Akces-Med employee or at specialized medical store!


AKCES-MED. Ltd. reserve the right to introduce technical and trading changes in the content of the instruction without warning.



Product marked with the CE sign is Class I medical device, of rule 1, consistent with the requirements of Regulation (EU) 2017/745 of the European Parliament and of the Council of 5 April 2017 on medical devices.



Akces-Med. Sp. z o.o. Company introduced quality management system ISO 13485 regarding production, sales and service. The system is certified by Det Norske Veritas.



CONTENTS

1. The purpose of user manual.....	5
2. Indications and contrindications for use.....	5
3. General characteristics of chair.....	6
3.1 Standard equipment.....	6
3.2 Additional equipment.....	7
4. Size table.....	9
5. Description how to use chair.....	10
6. Additional equipment.....	12
6.1 Head stabilizing belt.....	12
6.2 H harness.....	14
6.3 Hexagon Pro Headrest.....	14
6.4 Tray.....	15
6.5 Soft cover for tray.....	16
6.6 Tray for manual therapy.....	16
6.7 6 points harness.....	17
6.8 Self-leveling tray.....	18
7. The use of chair.....	19
7.1 Preparation of the patient.....	19
7.2 How to use chair.....	20
7.3 Sitting position.....	21
7.4 How to use vest.....	22
8. Safety rules.....	25
9. Terms of warranty.....	27
10. Maintenance and cleaning.....	28
11. Labelling.....	29



INTRODUCTION

Positioning chair JUMBO™ is used for initial upright standing of children in the sitting position. It is made of ecologic wood and therefore it is eco-friendly.

Despite its simplicity, it perfectly fulfils its function. It is safe for spastic as well as flaccid children with decreased muscle tone. Adjustable side supports help in correcting postural problems and, moreover, this chair may be beneficial regarding orthopaedic disorders.

It has a safety vest which is equipped with innovative Hold & Pull™ system thanks to which the child is both quick and precisely secured in this chair.

Each product is hand painted on water base paints. Size 3 thanks to the quick folding system of the footrest makes it easy to place and remove the person from the chair.

Remember to read this user manual carefully. You will find not only useful information but also guidelines regarding safe and effective use of the product.

If you have any questions or remarks, do not hesitate to contact with us:

Medical consultant: mobile +48 508 382 509

Akces-MED Sp. z o.o.: ph. +48 17 864 04 77

e-mail: export@akces-med.com

Thank you for purchasing our product.



Before using the product, user is obliged to familiarize himself/herself with user manual. Remember that complying with guidelines is highly important. It assures safety and extends durability as well as aesthetics of the device.

1. THE PURPOSE OF USER MANUAL



The instruction manual contains basic information necessary to properly prepare the chair before use, use the chair, maintain and clean the chair.

This user manual should be kept in an easily accessible place. The manual is intended for people who look after disabled users, as well as for doctors and physiotherapists handling the chair. Before using the chair for the first time, the user (or caregiver) is obliged to familiarize himself/herself with the user manual.

2. INDICATIONS AND CONTRINDICATIONS FOR USE

These medical devices are intended for people with orthopedic, neurological and cardiological diseases and for people after surgery, with musculoskeletal dysfunctions, who have not acquired the ability to sit independently or who have difficulties in adopting and maintaining the sitting position.

Both for flaccid people with reduced muscle tone and for people with spasticity. The device can also be really useful for people who require long-term relief of one or both lower limbs. It is an irreplaceable aid in the rehabilitation process, both in terms of movement and social integration. The device is great help during everyday activities such as rehabilitation but also during playing, studying or having meals. The selection of the appropriate size of the device depends on medical indications and anatomical parameters, regardless of the age of the user.

The device is recommended for people in the following cases:

- Cerebral palsy – various types and forms.
- Brain and spinal cord injuries with lower limbs paralysis and weakness, balance and motor coordination disorders with different etiology.
- Demyelinating disease (e.g. multiple sclerosis - SM).
- Meningocele.
- Muscles diseases with weakness and paralysis (dystrophy, myasthenia gravis, myositis).
- Genetic disorders.
- Degeneration and neurological diseases.
- Other condition connected with muscles weakness, paralysis and musculoskeletal disorders.
- After head and spinal cord injuries and spine trauma with paralysis and paresis.

Contraindications for sitting

- Critical condition of the user;
- Paralysis;
- Deep sedation;
- Unstable fractures with specific orthopedic recommendations, including spine fractures;
- Untreated deep vein thrombosis;
- Hemodynamic instability;
- Identified brain dysfunction when sitting upright;
- Severe arthritis of the cervical spine;
- Pulmonary embolism;
- Recent myocardial infarction in the last 24 hours;
- Fresh postoperative wounds or non-healing wounds in the back area, pelvic girdle area, hip joints and thighs;
- Users with mental disorders should not be left in the device without the supervision of a caregiver.




3. GENERAL CHARACTERISTICS OF CHAIR

3.1. Standard equipment

1. Frame with castors and brakes
2. Seat cushion
3. Backrest cushion
4. Independently adjustable chest supports
5. Independently adjustable pelvic supports
6. Hold&Pull vest
7. Abduction block
8. Foot rest with feet stabilizing belts



3.2. Additional equipment

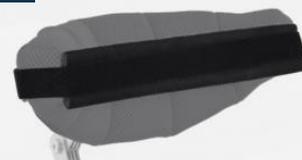
 <p>Safety</p> <p>SLK_002 Belt for moving the patients AM-P</p>	 <p>SLK_003 Soft cover for tray</p>	 <p>Stabilization</p> <p>SLK_101 Abduction-adduction thigh belts</p>
 <p>SLK_102 Head supporting belt</p>	 <p>SLK_104 Adjustable headrest</p>	 <p>SLK_114 H Harness</p>
 <p>SLK_123 Extended headrest</p>	 <p>SLK_123 Extended headrest</p>	 <p>SLK_340 Hexagon Pro™ BodyMap</p>
 <p>Comfort</p> <p>SLK_123 Extended headrest</p>	 <p>SLK_403 Tray</p>	 <p>SLK_429 Soft cover for the footrest</p>
 <p>SLK_431 Push handle</p>	 <p>SLK_448 Self-leveling tray</p>	 <p>Storage</p> <p>SLK_507 Oxygen tank holder</p>



SLK_015/016/020 TANGO
Wheel with brake



4. SIZE TABLE

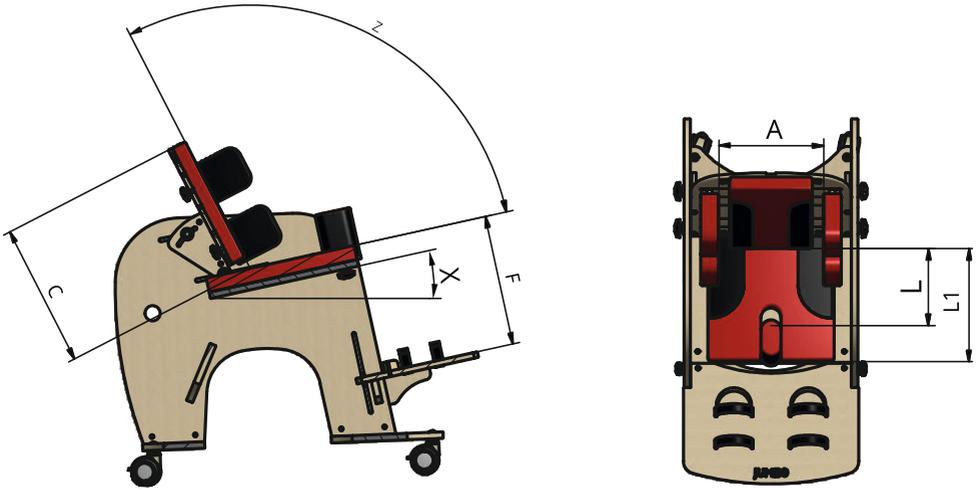

Symbol	Measurement	Unit	Size 1	Size 2	Size 3
W	Indicative user height*	[cm]	70 - 130	100 - 150	110 - 180
A	Seat width	[cm]	35	39	46
L	Seat depth	[cm]	13-31	19-38	29-54
L1	Distance from pommel to back rest	[cm]	0-24	3-29	8-45
C	Backrest height	[cm]	34	38	55
E	Backrest width	[cm]	17-27	22-32	22-35
F	Footrests length	[cm]	12-36	16-45	24-45
	Footplate length	[cm]	19	25	26
X	Seat tilt angle	[°]	10	10	10
Y	Backrest tilt angle	[°]	90-115	90-110	90-110
	Maximum user weight	[kg]	30	45	75

Weight and dimensions of the device		Size 1	Size 2	Size 3
Width	[cm]	50	54	60
Length	[cm]	82	100	120
Height	[cm]	76	95	105
Weight	[kg]	14	20	24,5

Note: Dimensional tolerance in the table is +1/-1 cm.

*This measurement cannot be the main parameter while choosing the product size.

5. DESCRIPTION HOW TO USE CHAIR

A. The adjustment of abduction block - The possibility of front-back adjustment. Abduction block prevents from falling out from the chair.

B. The adjustment of backrest tilt angle - backrest tilt angle depends on the type on dysfunction

C. The adjustment of seat depth - loosen knob in order to adjust the depth of seat B. The possibility of front-back adjustment


D. The adjustment of footrest height - The possibility of top-bottom adjustment. It is necessary to adjust the height of footrest so as that thighs rest on the seat.



1



E. The adjustment of chest pelottes - The possibility of side adjustment. It is also possible to adjust pelottes at any tilt angle. The adjustment of pelottes should be done according to the measurements of patient's chest.

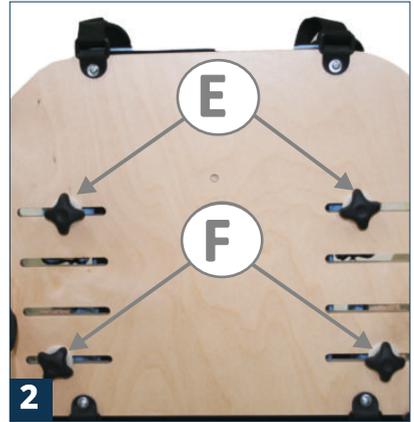

F. The adjustment of pelvic pelottes - The possibility of side adjustment. It is also possible to adjust pelottes at any tilt angle. The adjustment of pelottes should be done according to the measurements of patient's hips.

G. Vest

Connect clamps from vest with clamps from adjustable belts that are fastened both at the bottom and top of backrest (4 pcs.). Next, adjust vest to patient's body with the aid of belts.



It is highly important to adjust properly vest due to the fact that it protects the patient from falling out of the chair and, moreover, patient can move without freely. Vest is equipped with "hold&pull" system thanks to which all elements are precisely adjusted to patient. This system is helpful because the product is stable and child feels comfortable while sitting in this device.



Before using the vest, it is essential to familiarize yourself with the safety rules contained in the instruction. Information on how to safely use the VEST can be found on the page 22 of the instruction. Improper use and not obeying the safety rules may endanger the user's health and life.

CAUTION! Each time before using the harness check whether:


- The buckles do not unclip under the pressing force;
- The buckles and belts do not move as a result of incorrect fastening.





6. ADDITIONAL EQUIPMENT

6.1 REF SLK_102 Head supporting belt

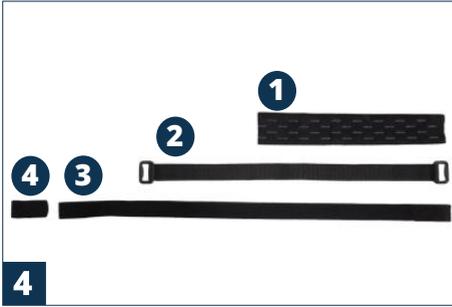

First, fit elements No. 1 and 3 to the user. To do this, cut them to the correct length.

5 6



After cutting the strips to the appropriate length, connect the strip No. 3 with the connector No. 4. (photo 7). Then connect the strip No. 1 with the strip No. 3 so that it is in the middle.





i

Then connect the two ends of the strip with the strip No. 2 in such a way that the indicated Velcro strip No. 2 is facing inwards.



i

Then we fasten the strap on the headrest.



6.2 **REF SLK_114** H Harness



Please look at point I so as to find out how to assembly vest (page 13). Initially, patient should not adjust vest tightly. Once vest is put on, it should be fastened with the aid of belts with plastic straps. Vest can be quickly unfastened.



Before using the vest, it is essential to familiarize yourself with the safety rules contained in the instruction. Information on how to safely use the VEST can be found on the page 22 of the instruction. Improper use and not obeying the safety rules may endanger the user's health and life.

CAUTION! Each time before using the harness check whether:

- The buckles do not unclip under the pressing force;
- The buckles and belts do not move as a result of incorrect fastening.

6.3 **REF SLK_104** Hexagon Pro Headrest



The headrest can be adjusted in 3 planes - height and depth adjustment (photo 14,15) and the width of the headrest (photo 16). Thanks to the modular structure, it is also possible to adjust the headrest to the shape of the user's head. This helps to properly position the head and improves the comfort of use. A properly stabilized and supported head significantly reduces the tension in the neck / nape muscles.



In order to adjust the height and depth of the headrest, loosen the indicated screws with an Allen key (photo 14), set the headrest in the desired position, tighten the screws firmly. **Make sure the headrest is locked in place.**



i

In order to adjust the width of the headrest, loosen the indicated screws with an Allen key (photo 16), set the headrest in the desired position, tighten the screws firmly. **Make sure the headrest is locked in place.**

6.4. **REF SLK_403** Tray

Please follow these steps so as to mount tray:

- loosen knob D which adjusts tray (**look page 10, adjustment D**);
- insert tray in a way that its grips are situated between chair's side and cup;
- tighten firmly knobs.



17

18



6.5. REF SLK_003 Soft cover for tray

Please follow these steps so as to mount soft cover for tray:

- Adhere 5 adhesive Velcro tapes;
- Put soft cover in a way that its edges cover tray edges.



6.6 REF SLK_401 Tray for manual therapy

Tray for manual therapy is mounted instead of standard tray. If you want to mount it, please follow instructions - page 15.



6.7 REF SLK_125 6 points safety vest

Please follow these steps so as to mount **6 points vest**:

STEP 1. Put vest on the patient and then zip up both zipper and clamp situated at the front of the vest (fig.22-25); Adjust vest with the aid of Velcro tapes situated at the back of the vest (fig. 26, 27)



- Adjust vest with the aid of Velcro tapes situated at the back of vest.
- 6 points vest should be fastened in a place that is created for standard vest (page 11). So as to fasten it, use not only buckles but also fastening belt that should be threaded behind chair's backrest and fastened at the front of vest.



Before using the vest, it is essential to familiarize yourself with the safety rules contained in the instruction. Information on how to safely use the VEST can be found on the page 22 of the instruction. Improper use and not obeying the safety rules may endanger the user's health and life.

CAUTION! Each time before using the harness check whether:

- The buckles do not unclip under the pressing force;
- The buckles and belts do not move as a result of incorrect fastening.



6.8 **REF SLK_448** Self-leveling tray



There is a bag filled with granules attached to the bottom of the tray with Velcro. It has a special pocket which allows you to adjust the amount of the granules depending on your needs. **Attention! An additional bag with granules is available as an option.**



7. THE USE OF CHAIR



JUMBO™ chair has to be used with compliance to guidelines included in this user manual. Remember to use the product only with someone who is trained and knowledgeable. Do not forget to prepare both product as well as patient before using JUMBO™ chair.

7.1. Preparation of the patient

Before using the product, it is essential to make sure that:

- patient's outfit is light and comfortable sporty clothes are advisable;
- shoes should be comfortable and, moreover, they should stabilize ankle;
- due to hygienic reason and to avoid abrasion it is advisable for the patient to always wear clothes when using the device, skin must not be naked especially in places of regular contact with upholstery;
- drains, bags, catheters etc. if applied, have to be secured to function properly and not to disturb during using the product;
- if it is necessary for a patient to wear orthopedic supply (collar, corset, orthosis, shoes) if it is recommended by doctor.



Outfit should protect patient's skin from direct contact with upholstery as well as other parts of equipment.

Only doctor can make a decision concerning using any kind of orthopedic supply!

7.2. How to use chair

1. Before use it is necessary to:
 - Unfold the device;
 - Place the device on even ground;
 - Make sure that all parts are serviceable, correctly mounted and stable;
 - Block brakes;
 - Adjust the device to patient's measurements;
 - Undo vest, trunk belts etc so as to place easily the patient in the device;
 - Place patient in the device;
 - Fasten all elements which stabilize patient e.g. vest, trunk belts, feet stabilizing belts etc.;
 - Mount additional equipment e.g. tray.

2. In case of patients who have problem with bladder, it is necessary to put special cloth on seat. This cloth can be purchased in pharmacy or medical shops.



Before the product is used, it is highly necessary to make sure that all belts as well as safety equipment are correctly fastened as well as adjusted. What is more, check if they do not become undone due to the pressure and, moreover, make sure that clampings from adjustable elements are firmly tightened!

Equipment works correctly only when the device is adjusted according to patient's height as well as weight. Remember to take all these measurements into account while purchasing the product. Correct adjustment is the most important due to the fact that only then the product is safe. It is forbidden to force child to keep specific position because he/she will feel uncomfortable and it may lead to wrong posture.

7.3. How to use chair

The first use of the positioning chair **JUMBO™** usually takes place at a rehabilitation, neurology, neurosurgery or orthopedics center. It is especially important to correctly adjust each element of the chair to the user regarding their condition and taking into account existing contractures and deformations. The first use of the chair at home should be done with the help of qualified staff (physiotherapist, health nurse, properly prepared family members) after having read the instruction manual.



Incorrect chair adjustment can lead to such side effects as fainting, body deformities, joint overload, etc. If the abovementioned symptoms occur, stop using the chair immediately, take the user out of the chair and lay them down. If the undesirable symptoms persist, contact a physician immediately. If the symptoms have disappeared, inform the attending physician about this fact in order to make a decision about the further rehabilitation process.

The decision to use the positioning chair must always be made by the attending physician.

Adjusting the chair to the user should only be done by people who have been properly trained and have read the instruction manual.

7.4. How to use vest



The vest provides posture support for wheelchair users as well as patients sitting in positioning chairs or other rehabilitation seats. When properly used, the vest allows the patient to adopt the correct sitting position for a longer period of time. The design and shape of the vest make it possible for the patient to be free to move their upper limbs within the constraints of the patient. **If the vest is not used properly, it can pose a serious threat to the health and life of the patient!**

Possible threats incident to the use of the vest:

- 1) **If the lower vest straps are fastened too loosely, there is a risk that the vest will move upwards to the patient's neck, making it difficult to breathe** – always check the tension of the straps and set them in such a way that the lower edge of the vest is located near the lower abdomen of the patient.
- 2) **In a situation when the patient slips off the seat, the upper edge of the vest covers the patient's neck and blocks the trachea, making it difficult to breathe** – it is therefore necessary to ALWAYS use the accessories stabilizing the patient's pelvis, such as a pelvic belt, thigh abduction belts or an abduction block.
- 3) **There is a risk that the upper straps of the vest will press the patient's neck, blocking the trachea and making it difficult to breathe.** This might happen if the patient's body is improperly secured in the seat or stroller – it is then necessary to use the optional accessories of these devices and stabilize the patient's body using the lateral supports. If there is no possibility to use such accessories with the device and the patient's body cannot be properly stabilized, the device should be replaced with the one having such an option.
- 4) **The vest is fastened too tightly to the backrest and as a result the patient cannot breathe easily** – in this case the vest should be loosened in such a way that it is possible for the caregiver to insert a straightened hand between the vest and the patient's body. If, however, we want to stabilize the patient's body properly, we should use a dynamic orthopedic vest, e.g. a Flex-point vest, which does not cause the breathing difficulty for the patient.

Instructions for the proper use of the vest:

- 1) Make sure that the patient is sitting in the best possible position:
 - in the middle of the seat,
 - deeply in the seat in such a way that the patient's lumbar spine rests against the backrest.
- 2) Secure the patient's pelvis with, for example, a pelvic belt, thigh abduction belts or an abduction block.
- 3) Make sure that the side supports of the device, if used, are set in the correct position. It is required that the patients with the poor trunk control use the side supports. The side supports limit the lateral movements of the patient's body, which could lead to the compression of the vest straps on the neck of the patient.
- 4) Secure the vest:
 - fasten and adjust the lower straps of the vest, so that the lower edge of the vest is located near the lower abdomen of the patient,
 - fasten the horizontal strap of the vest (if present),
 - fasten the shoulder straps of the vest,
 - check if the buckles of the vest do not open under pressure.
- 5) Check the patient's position:
 - make sure that the vest cannot move by itself towards the patient's neck,
 - make sure that you can insert a straightened hand between the vest and the patient's body.

To prevent injuries and to minimize the risks associated with the use of the vest, the following rules should be followed:

- 1) The position of the vest **MUST** be checked each time after putting the patient in the seat.
- 2) Special attention should be paid to protecting the patient from falling forward, slipping off the seat or lifting the pelvis. The vest **MUST** be used with the accessories which will secure the patient's pelvis at all times (e.g. the pelvic belt, thigh abduction belts or the abduction block). The use of the vest cannot be considered separately but as a part of a general posture support system including supports such as pelvic belts, foot support, torso stabilization, thigh abduction belts, tilt-in-space position and reclining backrest.
- 3) Special attention should be paid to ensuring that the entire foot of the patient has stable support. If the device is not equipped with a foot support, the patient's feet must rest firmly against the ground.

- 4) It should be remembered that any change of the inclination angle of the backrest, seat, foot support or tilt-in-space function might affect the effectiveness of the belts and supports!
- 5) Special attention should be paid to the use of stabilization elements or side supports. If the patient has poor trunk control, the side supports will limit the lateral movements, which could lead to the compression of the vest straps on the neck of the patient.
- 6) The mounting of the vest and adjusting it to the patient can only be carried out by a suitably trained person, who is familiar with the instructions for the use of the vest and the rules of its safe use.
- 7) Do not make any repairs or modifications to the vest on your own. In order to repair or replace any part of the vest, please contact the manufacturer.
- 8) Do not use a damaged or incomplete vest, as this poses a serious threat to the health and life of the patient!
- 9) Do not leave the patient in the device unattended!
- 10) The correctness of the use of the vest should be particularly controlled in accordance with the recommendations in case of children, patients with impaired memory or mentally ill.
- 11) Make sure that all people taking care of the patient are familiar with the rules of the safe use of the vest.

How to care for the vest:

The vest works effectively only if kept clean and maintained in accordance with the manufacturer's instructions. Before each use of the vest, check whether:

- 1) The vest straps are not frayed or worn. If so, have them exchanged for new ones,
- 2) The vest straps are not attached to the wheels of the device,
- 3) The buckles are not damaged. If so, have them exchanged for new ones,
- 4) The Velcro fastening holds firmly. If not, remove any dirt or hair from the Velcro, or have it replaced with a new one,
- 5) There have been no changes in the patient's height or weight from the moment the vest was adjusted to the patient,
- 6) The shoulder straps of the vest are adjusted so that they are not too loose or too tight,
- 7) The vest should be cleaned regularly with the use of warm soapy water and dried out of the direct sunlight and other sources of heat. The vest must always be dry before usage.

If you have any doubts or questions about the use of the vest, please contact your doctor or physiotherapist.

8. SAFETY RULES



JUMBO™ chair has to be used in compliance with guidelines in this user manual. duct as well as patient before using JUMBO™ chair.

It is highly important to consult either doctor or physiotherapist in order to make right decision concerning the choice of chair and its size. It is also essential to familiarize with the guidelines described in user manual before using the device.

1. Before use it is necessary to:

- make sure that there are no damages or different faults which could endanger patient's life; check if all parts are working and are correctly mounted and, moreover, check if they are not broken;
- check if all screws, knobs and all glued, sewed or tapped parts are tightened;
- check if brakes are operating correctly;
- check if buckles are operating correctly;
- always use safety belts, Velcro tapes should overlap min. 8cm;
- adjust the device according to patient's measurements and needs e.g. the adjustment of pelottes, footplate etc.;
- make sure that all movable parts and knobs for adjustments are stable and locked;
- secure patient with the aid of elements such as vest, foot stabilizing belts, pelottes, abduction block, headrest. It is highly important to secure patient because it safeguards him/her from falling out. If abduction contracture occurs, it is recommended to use abduction block in order to prevent ulcers between knees;

2. It is forbidden to use chair for different purposes that it is intended to.
3. It is forbidden to use chair when it is damaged or any part is missing.
4. It is forbidden to leave the patient unattended.
5. Chair should be used only when there is someone who is trained and knowledgeable.
6. It is forbidden to leave chair and the patient on unstable ground unattended, even if the brake is engaged.
7. It is forbidden to either go up or down the stairs; it doesn't matter if the patient is placed in the device or not.
8. It's important to make sure that patient doesn't stand on footer during either getting into or getting out the chair.
9. It is important to engage brake during getting into and getting out the chair.
10. Make sure that all limbs are not close to spokes or other adjustable elements.
11. Please pay your attention when approaching to sources of fire or sources of high temperature during using the device. Moreover, chair shouldn't be stored in rooms with high humidity.
12. Secure chair during transportation in order to avoid any possible damages. Manufacturer doesn't take responsibility for damages which appeared due to improper preparation of the device during transportation.
13. Before using the chair, remove all paper and plastic packaging. The packaging is not a toy! Keep away from children and animals.



Incorrect product adjustment can lead to such side effects as fainting, body deformities, joint overload, etc. If the abovementioned symptoms occur, stop using the product immediately, take the user out of the product and lay them down. If the undesirable symptoms persist, contact a physician immediately. If the symptoms have disappeared, inform the attending physician about this fact in order to make a decision about the further rehabilitation process. It is forbidden to place the patient in the device while being in car, bus or train.

The product contains small parts which children may swallow.

This device can be only used inside the buildings.



Do not use a product that has any signs of damage, tearing or wear. Only an undamaged product and proper use guarantee its right and safe working. If the product is damaged, discontinue use and contact the manufacturer.

Under no circumstances should an unqualified person repair or alter the product and its construction, as the health and safety of the user depend on it as well as it will lead to the loss of warranty.

The weight of user should not be bigger than maximal weight described on page 9 where you will find information regarding this issue.

Serious incidents involving this device should be reported both to manufacturer and to the competent authority in your country.

9. TERMS OF WARRANTY

- **Akces-MED Sp. z o. o** sells products free from manufacturing defects or faults.
- Manufacturer gives the purchaser **24-month** guarantee from the date of purchase. All defects revealed during warranty period will be repaired free of charge.
- All defects which appear after warranty period can be repaired only when the user will pay for it. This rule doesn't apply to refunded products - user can ask National Health Refund for refund.
- The chair is covered by a **36-month** warranty on the territory of Canada – the details of the rights resulting from the extended warranty are regulated by the warranty card.
- Manufacturer claims that the product can be used for **36-months**. User can use this product after this period only when he/she will send the device to manufacturer so as to service it. Next, manufacturer determines again how long the product can be used and, moreover, the date of the next service will be determined.
- If product is damaged, please contact our dealer or the **Akces-MED sp. z o. o**. Customer Service Department (ph. 17/864 04 70, e-mail: export@akces-med.com).

10. MAINTENANCE AND CLEANING

The positioning chair **JUMBO™**, which is a medical device, should always be kept clean and should be used in accordance with the manufacturer's instructions. The chair should be kept in a clean, dry and ventilated room. Maintenance and cleaning must be done at least once a month. Periodic cleaning and maintenance of the chair is essential to keep its proper functioning and safety.

Recommendations for cleaning the upholstery and other elements of the seat:

1. Wash with warm water using a soft cloth and mild cleaners.
2. Make sure the cloth is not too wet, as this may enlarge the stain and damage the upholstery or foam inside the upholstery.
3. Remember to remove excess moisture from the upholstery before the next cleaning.
4. After cleaning the stains, the upholstery should be rinsed with lukewarm water and dried with a clean cloth.
5. You must not soak the upholstery.
6. The upholstery must not get wet during cleaning.
7. Do not use hard brushes for cleaning the upholstery.
8. Do not clean the upholstery with strong chemicals, e.g. solvents or chlorine-based caustics.
9. Do not clean, replace any elements or maintain the chair during use.
10. Metal and plastic elements should be cleaned by hand with suitable cleaners, after having read the recommendations of the manufacturer of the given cleaner.



Remember that upholstery has to be always dry before using!
The manufacturer of the positioning chair, Akces-MED Sp. z o. o., is not responsible for any damages caused by using unsuitable cleaners.

Before using it is necessary to:

- clean wheels (in case they are mounted);
- check if brake stops turning wheel (in case they are mounted);
- make sure that all wooden parts e.g. tray don't have splinters;
- check if chair construction is free of breaks or any kinds of deformities;
- check if all movable parts are working and all screws, nuts, knobs etc. are correctly tightened;
- check if belts, vests, trunk belts, feet stabilizing belts etc are not frayed;
- check if buckles and clamps work correctly.



The manufacturer is only responsible for hidden defects or technical damage caused during the correct use of the chair. The manufacturer takes full responsibility for the proper functioning of the chair only when the user strictly follows the instruction of use.

In case of any damage, please contact the authorized retailer, where the chair was purchased, or the Akces-MED sp. z o. o. Customer Service Department.





TECHNICAL INSPECTION

Technical inspections should be performed regularly. Before servicing, the product should be thoroughly cleaned to reveal any hidden damage.

Frequency	What should be checked? What should be done?	Remarks
Before each use.	<p>General condition of the product.</p> <p>Check:</p> <ul style="list-style-type: none"> the entire product for any visible damage, cracks or mechanical defects,, if the product complete, if all bolts, screws, knobs, nuts and other elements of the construction are complete and tightened.. 	In case of any damage or defects, discontinue the use of the product and contact your Supplier/Distributor or the Manufacturer.
	<p>Wheels and brakes.</p> <p>Check:</p> <ul style="list-style-type: none"> if the wheels are properly mounted and if they are not damaged, if the brake is blocking the spinning wheel, if the wheels are not dirty. If necessary, clean the wheels. 	In case of any damage or defects, discontinue the use of the product and contact your Supplier/Distributor or the Manufacturer.
	<p>Fastening of the construction elements.</p> <p>Check all the mechanisms of the product and its moving parts. Check in particular:</p> <ul style="list-style-type: none"> if the seat is properly mounted (if applicable), if the wheels are properly mounted (if applicable), if the elements securing the user are properly mounted and if they work well (if applicable), if all the moving parts are complete, work properly, do not jam, if the adjustment mechanisms of the following elements work properly (if applicable): headrest, backrest, seat, abduction block, armrests, footrests. 	In case of any damage or defects, discontinue the use of the product and contact your Supplier/Distributor or the Manufacturer.
	<p>Upholstery elements.</p> <p>Check:</p> <ul style="list-style-type: none"> if there is any damage, tears, rips, loose seams or deformations on the upholstery elements, if the stabilizing straps, vests or safety belts are not frayed or twisted and if the buckles work properly, if the stabilizing straps, vests or safety belts work correctly and do not unfasten under pressure or when pulled. 	In case of any damage or defects, discontinue the use of the product and contact your Supplier/Distributor or the Manufacturer.
Once a week.	<p>Product cleaning.</p> <p>If the frame and upholstery get dirty (dusty, muddy, etc.) during everyday use, wipe them with a damp cloth without detergents. Remove dirt (e.g. hair, food remains, etc.) from the moving parts of the product.</p>	The product should be cleaned when necessary, but at least once a week. Do not use any chlorine based cleaners or methylated spirit. Before using the product, check if the upholstery is dry.



Frequency	What should be checked? What should be done?	Remarks	
Once a month.	Wheel axles, quick connectors (if applicable).	<p>Check:</p> <ul style="list-style-type: none"> if the wheels are rolling and if they are not loose. To maintain the wheels, apply a small amount of a preservative-lubricant between the axle and the wheel hub. Check if you can easily remove and attach the wheels. 	<p>Clean the wheels when dirty.</p> <p>In case of any damage or defects, discontinue the use of the product and contact your Supplier/Distributor or the Manufacturer.</p>
	Product construction connectors (welding, threading, soldering)	<p>Check:</p> <ul style="list-style-type: none"> the condition of the product frame in the places of joining (welds, threads, soldering). 	<p>In case of any damage or defects, discontinue the use of the product and contact your Supplier/Distributor or the Manufacturer.</p>
	Tires/innertubes (if applicable).	<p>Check:</p> <ul style="list-style-type: none"> tire wear condition. Check for visible damage. Check tire pressure (if applicable). 	<p>If the tire pressure is too low, inflate them to the correct level.</p> <p>In case of any damage or defects, discontinue the use of the product and contact your Supplier/Distributor or the Manufacturer.</p>
Once every 6 months.	Construction moving parts.	<p>Check:</p> <ul style="list-style-type: none"> if the moving parts of the construction have not been damaged. Maintain them using a proper cleaning agent. 	<p>In case of any damage or defects, discontinue the use of the product and contact your Supplier/Distributor or the Manufacturer.</p>
	Product labeling.	<p>Check:</p> <ul style="list-style-type: none"> if the marking and labels are readable. 	<p>In case of any damage or defects, discontinue the use of the product and contact your Supplier/Distributor or the Manufacturer.</p>
After the life time of the product finishes.	Detailed product check.	Check the product.	<p>The manufacturer specifies the life time of the product, which is given in the user manual. After the given period, the user may use the product only if it is sent back to the manufacturer to be checked first. After that, the manufacturer will re-define the life time of the product and the date of the next check.</p>

The list of all spare parts is available for download after selecting a product on www.akces-med.com.

11. LABELLING

11.1 SYMBOLS

- Declaration that the product meets the essential requirements
- Catalog number
- Serial number
- Please read the manual instructions before use
- Do not iron
- The product does not contain latex.
- Store in a dry place
- Careful! delicate content
- Protect from sunlight
- Storage temperature limitation
- Relative humidity storage
- Do not chlorinate
- Do not dry in a drum dryer

- Do not bleach
- Dry vertically
- Prohibition of use without fastened safety belts
- Prohibition to leave the patient without care during use of the product
- Product designed for indoor use
- Manufacturer
- Production date
- You need to read the additional information.
- You need to press the button shown in the photo.
- You need to use the tools indicated in the assembly description.
- You need to take special precautions.

11.2. EXAMPLE OF IDENTIFICATION PLATE

QR code - after scan you are directed to the website of the product

MANUFACTURER ADDRESS

MAKSYMALNE DOPUSZCZALNE OBCIĄŻENIE WYROBU

Serial number in the form of a bar code

Serial number

Name of product in polish

Name of product in English

Date of production

Labeling - look above

AKCESMED
www.akces-med.com

SLONIK 1
FOTELK REHABILITACYJNY

JUMBO 1
POSITIONING CHAIR

Akces-MED Sp. z o.o.
Jasionka 955B
38-002 JASIONKA
POLAND

05.2014

MAX LOAD: 25 kg


SLK 001/U/1/AA

MANUFACTURER



Akces-MED Sp. z o.o.

Jasionka 955B
36-002 Jasionka
tel. (17) 864 04 70
e-mail: export@akces-med.com
BDO: 000031619

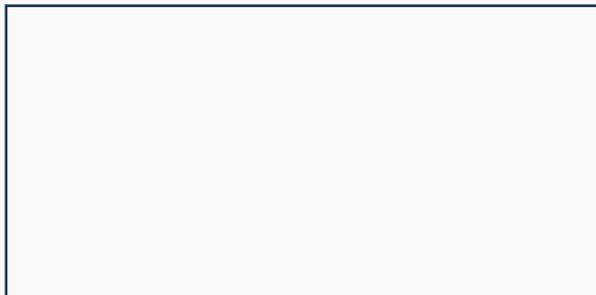

Authorised Dealer



akces-med.com

Date of issue: 01.04.2009
The last update: 20.05.2021
© Sławomir Wroński 2021